



Human Fibulin-1 ELISA Kit

User's Manual

For Research Use Only, Not for use in diagnostic procedures

ELISA Kit for Measuring Human Fibulin-1

CircuLex Human Fibulin-1 ELISA Kit

Cat# CY-8094

| | |
|--|-------|
| Intended Use..... | 1 |
| Storage..... | 1 |
| Introduction..... | 2 |
| Principle of the Assay..... | 2-3 |
| Materials Provided..... | 3 |
| Materials Required but not Provided..... | 4 |
| Precautions and Recommendations..... | 5 |
| Sample Collection and Storage..... | 6 |
| Detailed Protocol..... | 7-8 |
| Calculations..... | 9 |
| Measurement Range..... | 9 |
| Troubleshooting..... | 9 |
| Reagent Stability..... | 9 |
| Assay Characteristics..... | 10-12 |
| Example of Test Results..... | 13 |
| References..... | 14-15 |
| Related Products..... | 15 |

Intended Use

The CycLex Research Product **CircuLex Human Fibulin-1 ELISA Kit** is used for the quantitative measurement of human Fibulin-1 in plasma, cell culture supernatant and other biological media.

This assay kit is for research use only and not for use in diagnostic or therapeutic procedures.

Storage

- Upon receipt store all components at 4°C.
- Don't expose reagents to excessive light.

Introduction

Fibulin-1 is the first described member of a seven-gene family of extracellular matrix (ECM) proteins that have a common structural signature consisting of a series of repeated EGF-like domains followed by a fibulin-type module at its carboxyl terminus (1, 2). Fibulin-1 is a secreted glycoprotein that is an intercellular component of a wide range of connective tissues (3, 4). In blood vessel walls, fibulin-1 is a component of elastic lamina and ECM fibers that surround smooth muscle cells and underlie the endothelium. Although its actual function remains to be elucidated, fibulin-1 has been suggested to be involved in cell adhesion, migration, proliferation, and malignant transformation through binding to many ECM proteins, including laminin, fibrinogen, fibronectin, nidogen-1, endostatin, β -amyloid precursor protein and proteoglycans, aggrecan, versican (5-11), receptors and growth factors (12, 13). In addition, fibulin-1 has been found to bind to the plasma protein fibrinogen and to incorporate into fibrin clots formed in vitro and in vivo (14). Targeted inactivation of fibulin-1 gene in mice caused dilation and ruptures in the endothelial lining of small blood vessels (15), indicating that fibulin-1 was important in the stabilization of blood vessel walls.

Fibulin-1 is one of a few ECM proteins normally found in blood in high concentrations (16). It was reported that plasma fibulin-1 concentrations increased in T2DM patients with prevalent cardiovascular disease destined for vascular surgery (17) as well as in asthmatics (18).

Principle of the Assay

The CycLex Research Product **CircuLex Human Fibulin-1 ELISA Kit** employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for human Fibulin-1 is pre-coated onto a microplate. Standards and samples are pipetted into the wells and the immobilized antibody binds any human Fibulin-1 present. After washing away any unbound substances, an HRP conjugated antibody specific for human Fibulin-1 is added to the wells. Following a wash to remove any unbound antibody HRP conjugate, the remaining conjugate is allowed to react with the substrate H_2O_2 -tetramethylbenzidine. The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured at 450 nm. The absorbance is proportional to the concentration of human Fibulin-1. A standard curve is constructed by plotting absorbance values versus human Fibulin-1 concentrations of calibrators, and concentrations of unknown samples are determined using this standard curve.

Summary of Procedure

Add 100 μ L of diluted samples to the wells
↓ Incubate for 1 hour at room temp.
Wash the wells
↓
Add 100 μ L of HRP conjugated anti-human Fibulin-1 antibody
↓ Incubate for 1 hour at room temp.
Wash the wells
↓
Add 100 μ L of Substrate Reagent
↓
Add 100 μ L of Stop Solution
↓
Measure absorbance at 450 nm

Materials Provided

All samples and standards should be assayed in duplicate. The following components are supplied and are sufficient for the one 96-well microplate kit.

Microplate: One microplate supplied ready to use, with 96 wells (12 strips of 8-wells) in a foil, zip-lock bag with a desiccant pack. Wells are coated with anti-human Fibulin-1 antibody as a capture antibody.

10X Wash Buffer: One bottle containing 100 mL of 10X buffer containing 2% Tween®-20

Dilution Buffer: One bottle containing 50 mL of 1X buffer; use for Human Fibulin-1 Standard and sample dilution. Ready to use.

Human Fibulin-1 Standard: One vial containing 270 ng of lyophilized recombinant human Fibulin-1.

HRP conjugated Detection Antibody: One bottle containing 12 mL of HRP (horseradish peroxidase) conjugated anti-human Fibulin-1 antibody. Ready to use.

Substrate Reagent: One bottle containing 20 mL of the chromogenic substrate, tetra-methylbenzidine (TMB). Ready to use.

Stop Solution: One bottle containing 20 mL of 1 N H₂SO₄. Ready to use.

Materials Required but not Provided

- **Pipettors:** 2-20 μ L, 20-200 μ L and 200-1000 μ L precision pipettors with disposable tips
- **Precision repeating pipettor**
- **Orbital microplate shaker**
- **Microcentrifuge and tubes** for sample preparation
- **Vortex mixer**
- **Microplate washer:** optional (Manual washing is possible but not preferable)
- **Plate reader:** capable of measuring absorbance in 96-well plates at dual wavelengths of 450/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. The plate can also be read at a single wavelength of 450 nm, which will give a somewhat higher reading.
- **Software package facilitating data generation and analysis :**optional
- **500 or 1000 mL graduated cylinder**
- **Reagent reservoirs**
- **Deionized water of the highest quality**
- **Disposable paper towels**

Precautions and Recommendations

- Allow all the components to come to room temperature before use.
- All microplate strips that are not immediately required should be returned to the zip-lock pouch, which must be carefully resealed to avoid moisture absorption.
- Do not use kit components beyond the indicated kit expiration date.
- Use only the microtiter wells provided with the kit.
- Rinse all detergent residues from glassware.
- Use deionized water of the highest quality.
- Do not mix reagents from different kits.
- The buffers and reagents in this kit may contain preservatives or other chemicals. Care should be taken to avoid direct contact with these reagents.
- Do not mouth pipette or ingest any of the reagents.
- Do not smoke, eat, or drink when performing the assay or in areas where samples or reagents are handled.
- Dispose of tetra-methylbenzidine (TMB) containing solutions in compliance with local regulations.
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide.
- Wear gloves and eye protection when handling immunodiagnostic materials and samples of human origin, and these reagents. In case of contact with the Stop Solution and the Substrate Solution, wash skin thoroughly with water and seek medical attention, when necessary.
- **Biological samples may be contaminated with infectious agents. Do not ingest, expose to open wounds or breathe aerosols. Wear protective gloves and dispose of biological samples properly.**
- **CAUTION: Sulfuric Acid is a strong acid. Wear disposable gloves and eye protection when handling Stop Solution.**

Sample Collection and Storage

Plasma: Collect plasma using EDTA-Na₂ as the anticoagulant. If possible, collect the plasma into a mixture of EDTA-Na₂ and Futhan5 to stabilize the sample against spontaneous *in vitro* complement activation. Immediately centrifuge samples at 4°C for 15 minutes at 1,000 x g. Assay immediately or store samples on ice for up to 6 hours before assaying. Aliquots of plasma may also be stored at below -70°C for extended periods of time. Avoid repeated freeze-thaw cycles.

Note: Citrate plasma has not been validated for use in this assay.

Serum: Use a serum separator tube and allow samples to clot for 60 ± 30 minutes. Centrifuge the samples at 4°C for 10 minutes at 1,000 x g. Remove serum and assay immediately or store samples on ice for up to 6 hours before assaying. Aliquots of serum may also be stored at below -70°C for extended periods of time. Avoid repeated freeze-thaw cycles.

Cell culture supernatant: Remove any particulates by centrifugation and assay immediately or aliquot and store samples at below -70°C. Avoid repeated freeze-thaw cycles.

Other biological samples: Remove any particulates by centrifugation and assay immediately or aliquot and store samples at below -70°C. Avoid repeated freeze-thaw cycles.

Detailed Protocol

The CycLex Research Product **CircuLex Human Fibulin-1 ELISA Kit** is provided with removable strips of wells so the assay can be carried out on separate occasions using only the number of strips required for the particular determination. Since experimental conditions may vary, an aliquot of the human Fibulin-1 Standard within the kit should be included in each assay as a calibrator. Disposable pipette tips and reagent troughs should be used for all liquid transfers to avoid cross-contamination of reagents or samples.

Preparation of Working Solutions

All reagents need to be brought to room temperature prior to the assay. Assay reagents are supplied ready-to-use, with the exception of **10X Wash Buffer** and **Human Fibulin-1 Standard**.

1. Prepare a working solution of Wash Buffer by adding 100 mL of the **10X Wash Buffer** to 900 mL of deionized (distilled) water (ddH₂O). Mix well. Store at 4°C for two weeks or -20°C for long-term storage.
2. Reconstitute **Human Fibulin-1 Standard** with **0.45 mL** of ddH₂O. The concentration of the human Fibulin-1 in vial should be **600 ng/mL**, which is referred as a **Master Standard** of human Fibulin-1.

Prepare Standard Solutions as follows:

Use the **Master Standard** to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 60 ng/mL standard (Std.1) serves as the highest standard. The **Dilution Buffer** serves as the zero standard (Blank).

| | Volume of Standard | Dilution Buffer | Concentration |
|-------|--------------------------------------|-----------------|---------------|
| Std.1 | 60 µL of Master Standard (600 ng/mL) | 540 µL | 60 ng/mL |
| Std.2 | 300 µL of Std. 1 (60 ng/mL) | 300 µL | 30 ng/mL |
| Std.3 | 300 µL of Std. 2 (30 ng/mL) | 300 µL | 15 ng/mL |
| Std.4 | 300 µL of Std. 3 (15 ng/mL) | 300 µL | 7.5 ng/mL |
| Std.5 | 300 µL of Std. 4 (7.5 ng/mL) | 300 µL | 3.75 ng/mL |
| Std.6 | 300 µL of Std. 5 (3.75 ng/mL) | 300 µL | 1.88 ng/mL |
| Std.7 | 300 µL of Std. 6 (1.88 ng/mL) | 300 µL | 0.94 ng/mL |
| Blank | - | 300 µL | 0 ng/mL |

Note: Do not use a Repeating pipette. Change tips for every dilution. Unused portions of Master Standard should be aliquoted and stored at below -70°C immediately. Avoid multiple freeze and thaw cycles.

Sample Preparation

- Serum and plasma samples require a 1,000-fold dilution.
- Cell culture supernatant samples may require 1- to 10-fold dilution.
- Other biological samples may require 1- to 100-fold dilution.

Standard Assay Procedure for Human Fibulin-1

1. Remove the appropriate number of microtiter wells from the foil pouch and place them into the well holder. Return any unused wells to the foil pouch, refold, seal with tape and store at 4°C.
2. Dilute samples with Dilution Buffer. (See "Sample Preparation" above.)
3. Pipette **100 µL** of **Standard Solutions (Std1-Std7, Blank)** and **diluted samples** in duplicates, into the appropriate wells.
4. Incubate the plate **at room temperature (ca.25°C) for 1 hour, shaking at ca. 300 rpm on an orbital microplate shaker.**
5. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
6. Add **100 µL** of **HRP conjugated Detection Antibody** into each well.
7. Incubate the plate **at room temperature (ca.25°C) for 1 hour, shaking at ca. 300 rpm on an orbital microplate shaker.**
8. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
9. Add **100 µL** of **Substrate Reagent** to each well. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with e.g. aluminum foil is recommended. Return Substrate Reagent to 4°C immediately after the necessary volume is removed
10. Incubate the plate **at room temperature (ca.25°C) for 10-20 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.** The incubation time may be extended up to 30 minutes if the reaction temperature is below than 20°C.
11. Add **100 µL** of **Stop Solution** to each well in the same order as the previously added Substrate Reagent.
12. Measure absorbance in each well using a spectrophotometric microplate reader at dual wavelengths of 450/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. Read the microplate at 450 nm if only a single wavelength can be used. Wells must be read within 30 minutes of adding the Stop Solution.

Note-1: Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

Note-2: Reliable standard curves are obtained when either O.D. values do not exceed 0.25 units for the blank (zero concentration), or 3.0 units for the highest standard concentration. The plate should be monitored at 5-minute intervals for approximately 30 minutes.

Note-3: If the microplate reader is not capable of reading absorbance greater than the absorbance of the highest standard, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine human Fibulin-1 concentration of off-scale samples. The readings at 405 nm should not replace the on-scale readings at 450 nm.

Calculations

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density. Plot the optical density for the standards versus the concentration of the standards and draw the best curve. The data can be linearized by using log/log paper and regression analysis may be applied to the log transformation. To determine the human Fibulin-1 concentration of each sample, first find the absorbance value on the y-axis and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the x-axis and read the corresponding human Fibulin-1 concentration. If the samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

1. The dose-response curve of this assay fits best to a sigmoidal 4-parameter logistic equation. The results of unknown samples can be calculated with any computer program having a 4-parameter logistic function. It is important to make an appropriate mathematical adjustment to accommodate for the dilution factor.
2. Most microtiter plate readers perform automatic calculations of analyte concentration. The calibration curve is constructed by plotting the absorbance (Y) of calibrators versus log of the known concentration (X) of calibrators, using the 4-parameter function. Alternatively, the logit log function can be used to linearize the calibration curve (i.e. logit of absorbance (Y) is plotted versus log of the known concentration (X) of calibrators).

Measurement Range

The measurement range is 0.94 ng/mL to 60 ng/mL. Any sample reading higher than the highest standard should be diluted with Dilution Buffer in higher dilution and re-assayed. Dilution factors need to be taken into consideration in calculating the human Fibulin-1 concentration.

Troubleshooting

1. The Human Fibulin-1 Standard should be run in duplicate, using the protocol described in the **Detailed Protocol**. Incubation times or temperatures significantly different from those specified may give erroneous results.
2. Poor duplicates, accompanied by elevated values for wells containing no sample, indicate insufficient washing. If all instructions in the **Detailed Protocol** were followed accurately, such results indicate a need for washer maintenance.
3. Overall low signal may indicate that desiccation of the plate has occurred between the final wash and addition of Substrate Reagent. Do not allow the plate to dry out. Add Substrate Reagent immediately after wash.

Reagent Stability

All of the reagents included in the CycLex Research Product **CircuLex Human Fibulin-1 ELISA Kit** have been tested for stability. Reagents should not be used beyond the stated expiration date. Upon receipt, kit reagents should be stored at 4°C, except the reconstituted Fibulin-1 Standard must be stored at below -70°C. Coated assay plates should be stored in the original foil bag sealed by the zip lock and containing a desiccant pack.


Assay Characteristics

1. Sensitivity

The limit of detection (defined as such a concentration of human Fibulin-1 giving absorbance higher than mean absorbance of blank* plus three standard deviations of the absorbance of blank: A blank + 3SD blank) is better than 0.23 ng/mL of sample.

* Dilution Buffer is pipetted into blank wells.

Typical Standard Curve

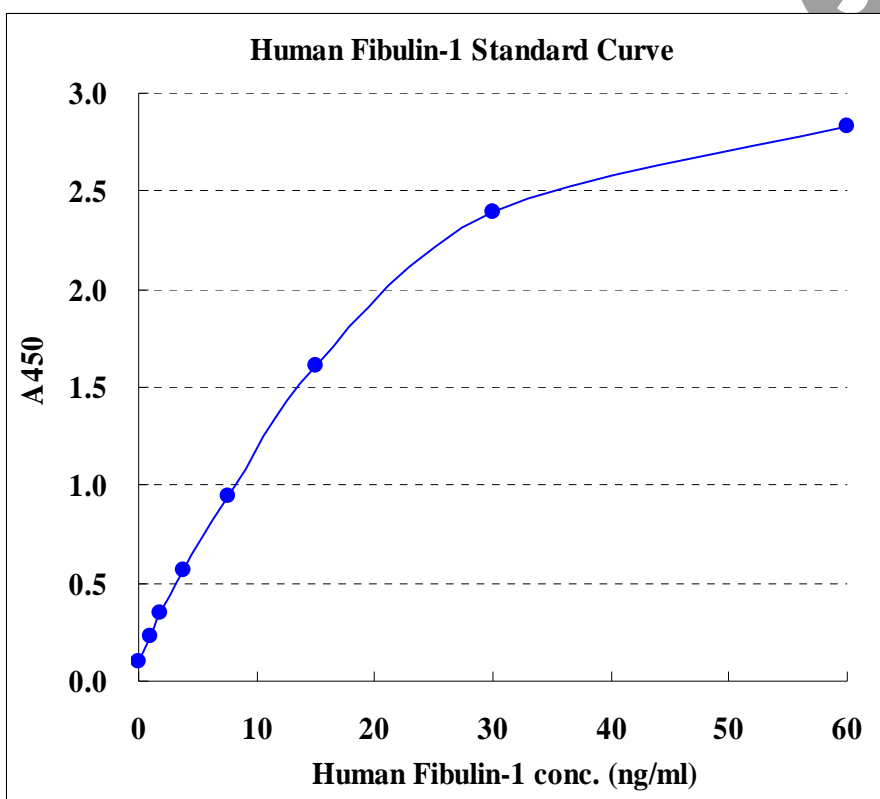

2. Precision

Intra-assay Precision (Precision within an assay)

Three samples of known concentration were tested sixteen times on one plate to assess intra-assay precision. Please note all samples are 1,000-fold diluted as stated in the Assay Procedure.

- Intra-assay (Within-Run, n=7) CV=4.5-5.1 %

| Human Fibulin-1 conc. (ng/ml) | | | |
|-------------------------------|-------------|-------------|-------------|
| | Sample 1 | Sample 2 | Sample 3 |
| 1 | 29.5 | 10.5 | 4.4 |
| 2 | 31.8 | 9.8 | 4.2 |
| 3 | 26.1 | 9.5 | 4.2 |
| 4 | 29.8 | 10.1 | 4.6 |
| 5 | 28.8 | 9.3 | 4.2 |
| 6 | 29.5 | 10.0 | 4.5 |
| 7 | 29.7 | 9.7 | 4.3 |
| 8 | 28.3 | 9.7 | 4.1 |
| 9 | 31.4 | 10.4 | 4.4 |
| 10 | 30.4 | 10.2 | 4.3 |
| 11 | 28.6 | 9.8 | 4.4 |
| 12 | 29.3 | 8.9 | 4.9 |
| 13 | 26.9 | 9.7 | 4.2 |
| 14 | 28.6 | 10.2 | 4.1 |
| 15 | 28.1 | 9.5 | 4.2 |
| 16 | 30.5 | 9.2 | 4.2 |
| MAX. | 31.8 | 10.5 | 4.9 |
| MIN. | 26.1 | 8.9 | 4.1 |
| MEAN | 29.2 | 9.8 | 4.3 |
| S.D. | 1.49 | 0.44 | 0.20 |
| C.V. | 5.1% | 4.5% | 4.7% |

Inter-assay Precision (Precision between assays)


Three samples of known concentration were tested in five separate assays to assess inter-assay precision. Please note all samples are 1,000-fold diluted as stated in the Assay Procedure.

- Inter-assay (Run-to-Run, n=5) CV=4.1-9.1 %

| Human Fibulin-1 conc. (ng/ml) | | | |
|-------------------------------|-------------|-------------|-------------|
| | Sample 1 | Sample 2 | Sample 3 |
| 1 | 31.2 | 10.7 | 5.1 |
| 2 | 27.1 | 11.2 | 5.1 |
| 3 | 26.2 | 9.1 | 4.7 |
| 4 | 24.8 | 10.5 | 4.7 |
| 5 | 26.1 | 10.2 | 5.0 |
| MAX. | 31.2 | 11.2 | 5.1 |
| MIN. | 24.8 | 9.1 | 4.7 |
| MEAN | 27.1 | 10.3 | 4.9 |
| S.D. | 2.45 | 0.78 | 0.20 |
| C.V. | 9.1% | 7.6% | 4.1% |

3. Linearity

Three biological samples were diluted with Dilution Buffer and assayed after dilution. The neat sample is set to 1. Please note all samples including the neat sample are 1,000-fold diluted as stated in the Assay Procedure. The results are summarized in the figure below.

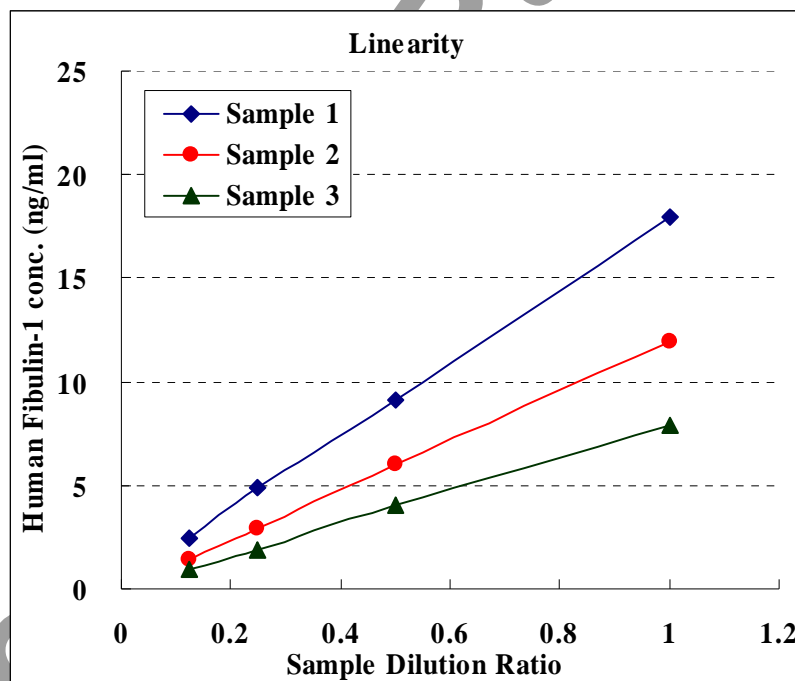

Example of Test Results

Fig.1 Human Fibulin-1 concentration in conditioned media of several cell lines


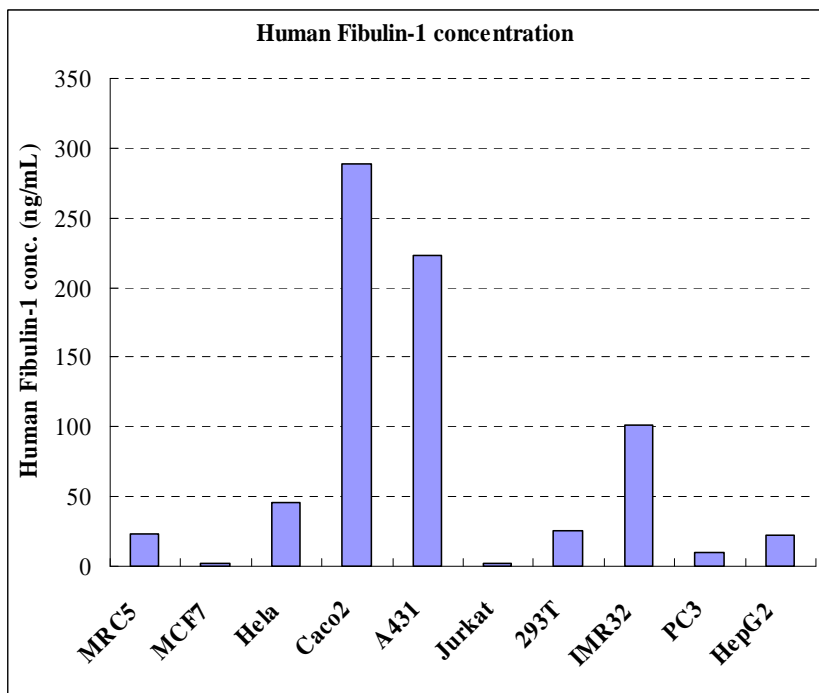


Fig.2 The correlation of Human Fibulin-1 concentrations in human plasma and serum

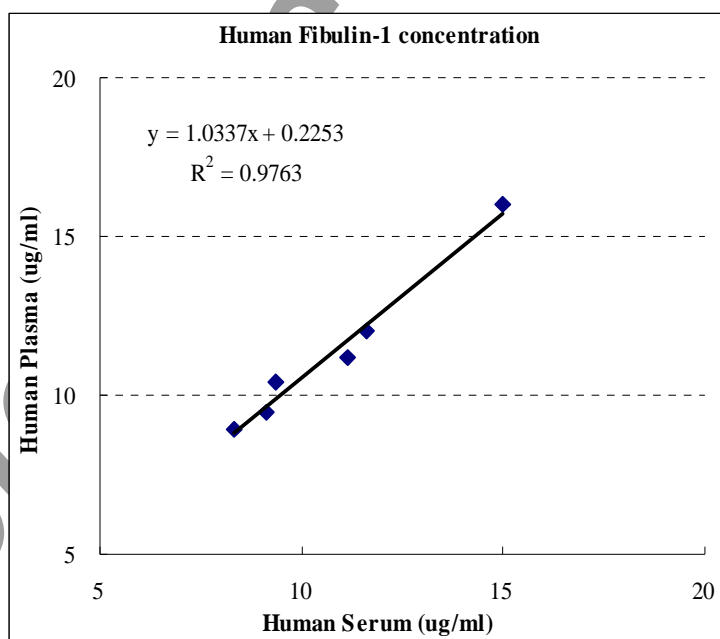

References

1. Argraves, WS, Greene LM, Cooley MA & Gallagher WM (2003) Fibulins: physiological and disease perspectives. *EMBO Rep.* 4, 1127-1131.
2. Chu ML, Tsuda T. (2004) Fibulins in development and heritable disease. *Birth Defects Res C Embryo Today* 72, 25-36
3. Kluge M, Mann K, Dziadek M, Timpl R (1990) Characterization of a novel calcium-binding 90-kDa glycoprotein (BM-90) shared by basement membranes and serum. *Eur J Biochem* 193, 65
4. Roark EF et al. (1995) The association of fibulin-1 with elastic fibers: An immunohistological, ultrastructural and RNA study. *J Histochem Cytochem* 43, 401
5. Timpl R and Brown JC (1994) The laminins. *Matrix Biol*, 14, 275-281.
6. Godyna, S., Diaz-Ricart, M., and Argraves, W. S. (1996) Fibulin-1 promotes platelet adhesion via a bridge of fibrinogen to the integrin $\alpha\text{IIb}\beta_3$. *Blood* 88, 2569-2577.
7. Tran H, VanDusen WJ and Argraves WS. (1997) The self-association and fibronectin-binding sites of fibulin-1 map to calcium-binding epidermal growth factor-like domains. *J. Biol. Chem.* 272, 22600-22606.
8. Aspberg A et al. (1999) Fibulin-1 is a ligand for the C-type lectin domains of aggrecan and versican. *J. Biol. Chem.* 274, 20444-20449
9. Miosge, N., Sasaki, T., and Timpl, R. (1999) Angiogenesis inhibitor endostatin is a distinct component of elastic fibers in vessel walls *FASEB J.* 13, 1743-1750.
10. Olin AI et al. (2001) The proteoglycans aggrecan and versican form networks with Fibulin-2 through their lectin domain binding. *J. Biol. Chem.* 276, 1253-1261
11. Ohsawa I, Takamura C, Kohsaka S. (2001) Fibulin-1 binds the amino-terminal head of beta-amyloid precursor protein and modulates its physiological function. *J Neurochem.* 76, 1411-20.
12. Timpl R, Sasaki T, Kostka G, Chu ML. (2003) Fibulins: a versatile family of extracellular matrix proteins. *Nat Rev Mol Cell Biol* 4, 479-489
13. Argraves WS, Dickerson K, Burgess WH, Ruoslahti E. (1989) Fibulin, a novel protein that interacts with the fibronectin receptor beta subunit cytoplasmic domain. *Cell.* 58, 623-9.
14. Tran H et al. (1995) The interaction of fibulin-1 with fibrinogen: A potential role in hemostasis and thrombosis. *J Biol Chem* 270, 19458.
15. Kostka G et al. (2001) Perinatal lethality and endothelial cell abnormalities in several vessel compartments of fibulin-1-deficient mice. *Mol Cell Biol* 21, 7025-7034
16. Argraves WS, Tran H, Burgess WH, Dickerson K. (1990) Fibulin is an extracellular matrix and plasma glycoprotein with repeated domain structure. *J Cell Biol* 111, 3155-64.

17. Cangemi C et al. (2011) Fibulin-1 is a marker for arterial extracellular matrix alterations in type 2 diabetes. Clin Chem.57, 1556-65.
18. Lau JY et al. (2010) Fibulin-1 is increased in asthma--a novel mediator of airway remodeling? PLoS One 5, e13360.

Related Products

- * CircuLex Human RBP4 ELISA Kit: Cat# CY-8072
- * CircuLex Human YKL-39 ELISA Kit: Cat# CY-8087
- * CircuLex Human YKL-40 ELISA Kit: Cat# CY-8088
- * CircuLex Human S100A12 ELISA Kit: Cat# CY-8058
- * CircuLex Human Chitotriosidase ELISA Kit: Cat# CY-8074

PRODUCED BY

CycLex Co., Ltd.
1063-103 Terasawaoka
Ina, Nagano 396-0002
Japan
Fax: +81-265-76-7618
e-mail: info@cyclex.co.jp
URL: <http://www.cyclex.co.jp>

CycLex/CircuLex products are supplied for research use only. CycLex/CircuLex products and components thereof may not be resold, modified for resale, or used to manufacture commercial products without prior written approval from CycLex Co., Ltd.. To inquire about licensing for such commercial use, please contact us via email.